



# 70u 70PSI Standard Config

Cytometer:	FACSriaII	User:	Administrator
Cytometer Name:	FACSriaIII	Institution:	
Serial Number:	P28200125	Software:	BD FACSDiva 6.1.3
Input Device:	Manual	Date:	4/23/2012 9:52:56 AM
Sheath Pressure:	70.00		
Nozzle Size:	70		
Window Extension:	2.00		


4001111 Laser  
(488nm)  
ESC

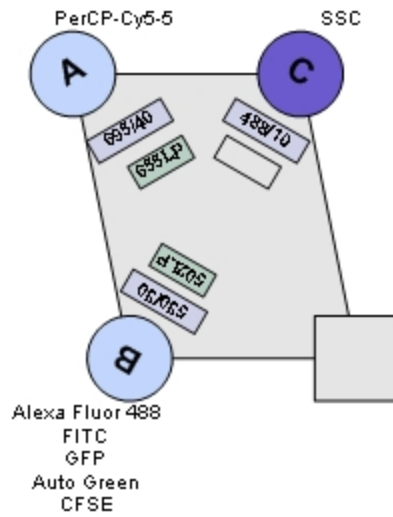


561nm Laser  
(561nm)

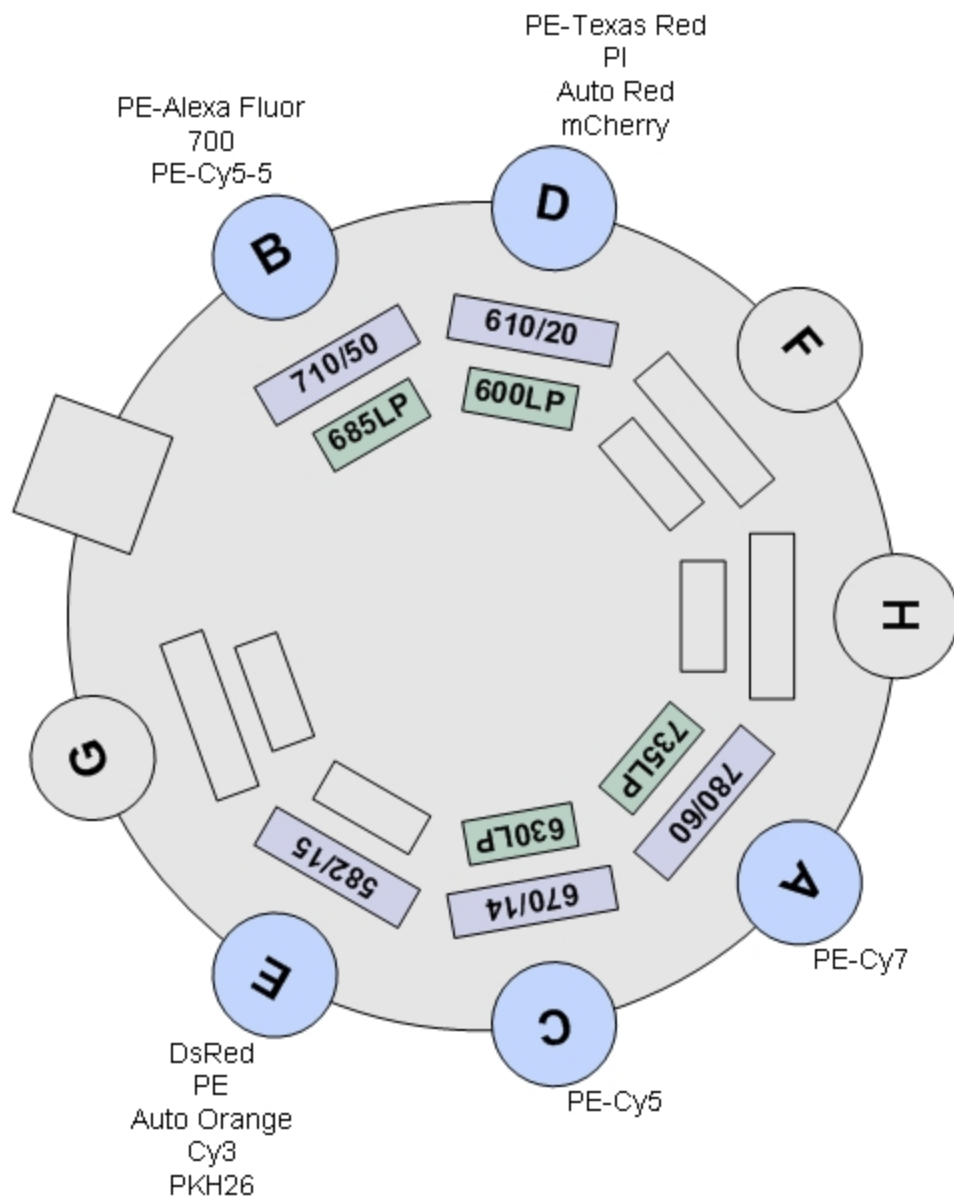

633nm Laser  
(633nm)

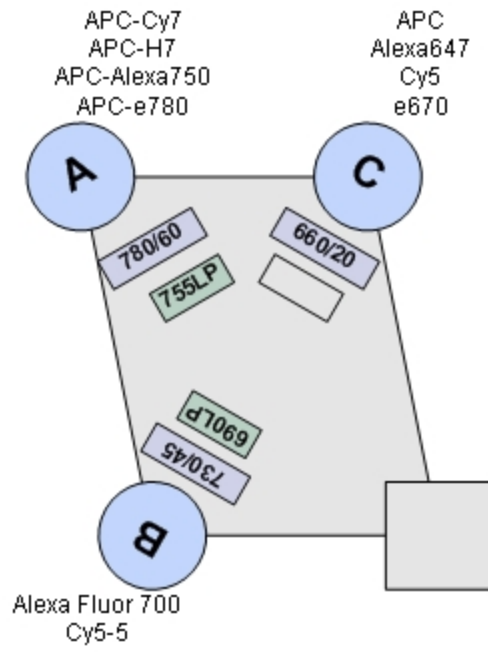

405nm Laser  
(405nm)

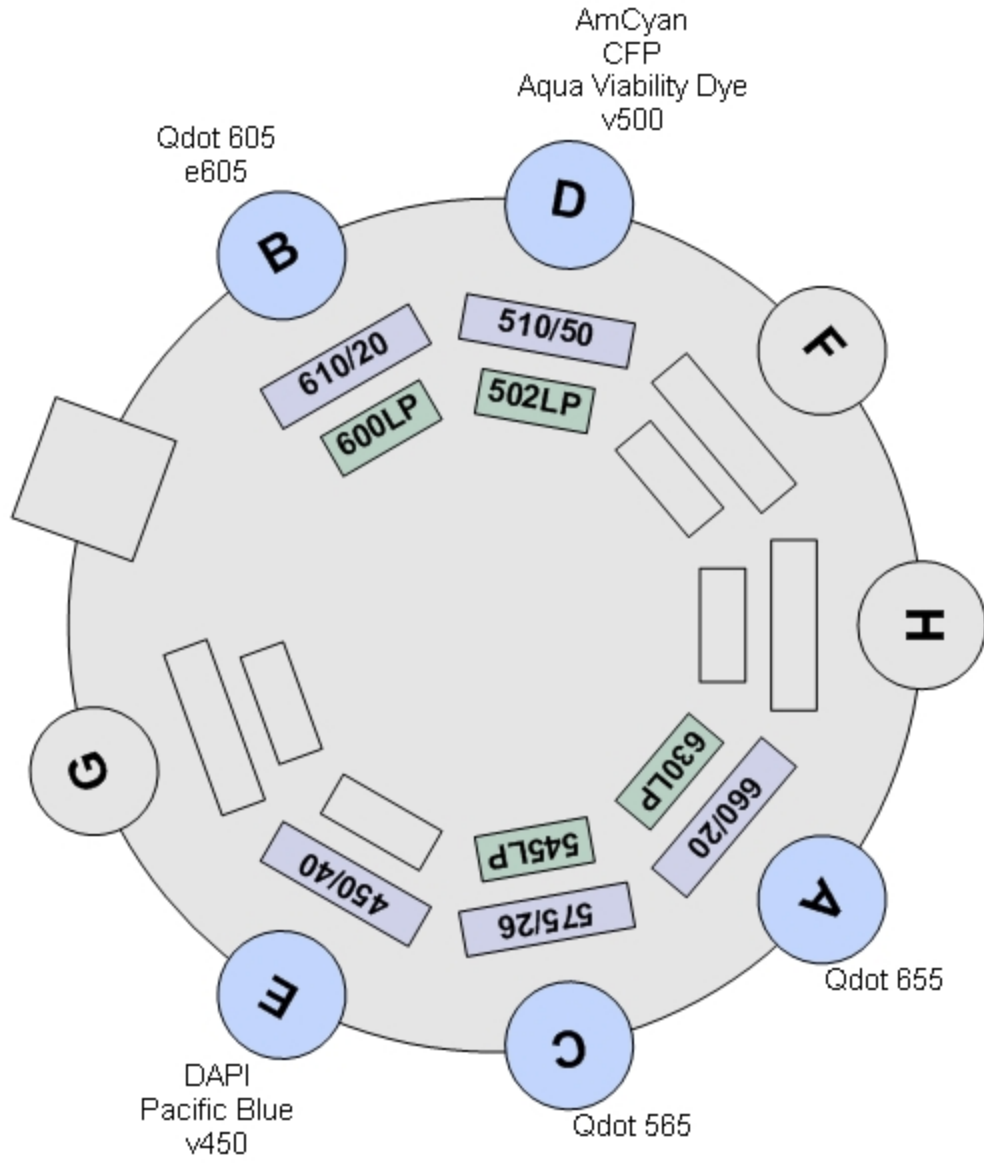

Comments: