



SEREF0 New config 6-Blue 6-Violet 0-UV 3-Red

| | | | |
|-------------------|-----------|--------------|----------------------|
| Cytometer: | LSRII | User: | Administrator |
| Cytometer Name: | LSRII | Institution: | |
| Serial Number: | H48300010 | Software: | BD FACSDiva 6.1.1 |
| Input Device: | Manual | Date: | 6/13/2018 2:33:17 PM |
| Window Extension: | 10.00 | | |


Blue Laser
(488nm)
FSC

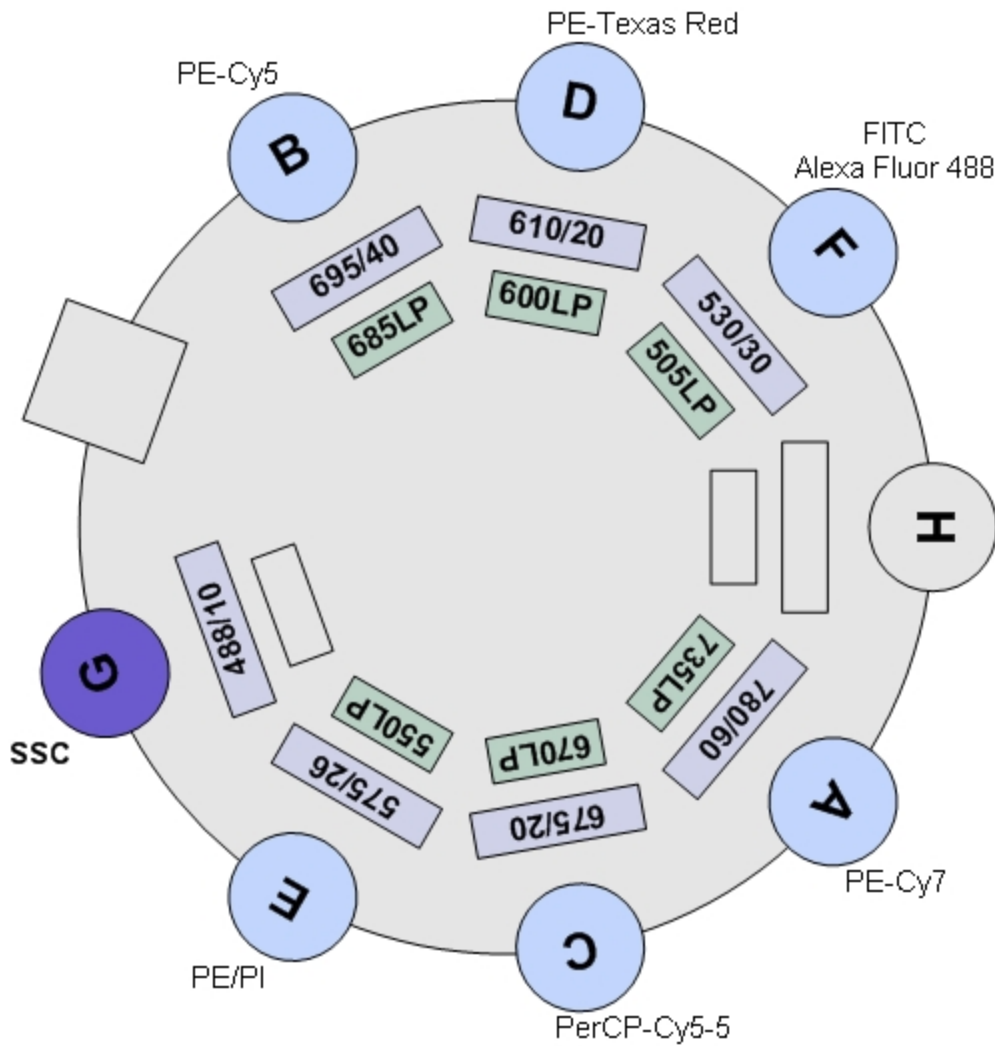

Red Laser
(633nm)

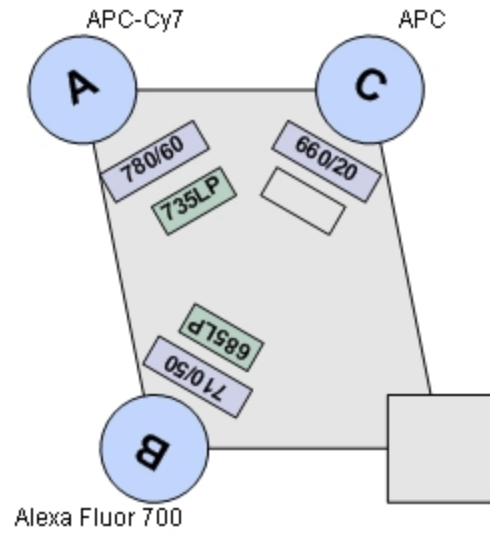

Violet Laser
(405nm)

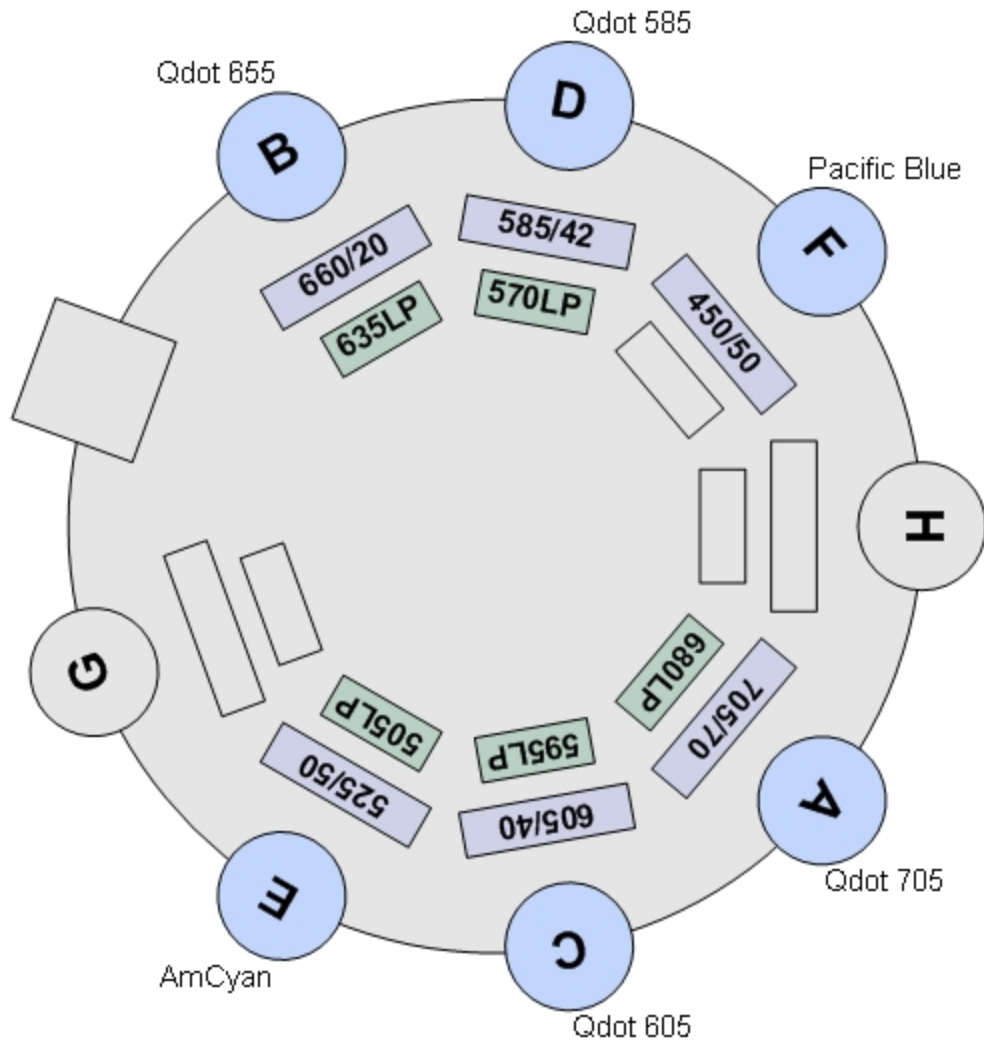

Comments: